

# INSPECTION REPORT

Customer:

**IAA**

Page 1/4

+ 0 appendix

Ref.: WS-PVC5893-A	Project: SLICER MAAT	File nb: 24906
Date: 26 Sep. 2024	Title: Inspection before coating	Order n: -
Project manager: LAPERE, M. Vincent	Piece: MAAT mirror Reference: 23160-112-F302 SN: 1	

pplicable documents. : (drawing, documents...) Indicate the issue	Drawing n° 23160-112-F302-A
Distribution list: Files, Customer	Original: QA

## Inspection before coating

Parameter	Requirement	Value	Compliance	Comment
Material	Fused Silica	Fused Silica	Yes	-
Length (mm)	42 +/-0.5	42.07	C	
Width (mm)	38 +/-0.5	38.17	C	
Thickness (mm)	20 +/-0.5	20.46	C	
Tangential Radius (along length)	104.151 mm +/-1%	104.16	C	
Sagittal Radius (along width)	93.812 mm +/-1%	94.60	C	
Wedge along Length	< 3arcmin (35µm over 40mm)	1.12 arcmin	C	
Wedge along width	< 3arcmin (35µm over 40mm)	1.24 arc min	C	
Clear aperture	20x20 centered	> 20x20 centered	C	
Shape error over CA	80nm RMS (Goal 40nm RMS)	48.3 nm RMS	C	
Aspect	60/40 (Goal 20/10)	Nothing to report	C	
Roughness	3nm RMS (Goal 1.5nm RMS)	0.69 nm RMS	C	

Control Result		Statement		
Compliant:	1	<input type="checkbox"/> under restriction	Accepted:	1
Non-compliant:	0	Request for waiver ref.:	Refused:	0
Observation:				
	Inspector	Project Manager	Quality Manager	
Date and Signature	30/09/2024	30/09/2024	30/09/2024	
	X Aurélie Monier	X Vincent LAPERE	X Richard Holowczak	
	Inspector	Project Manager	Quality	
	Signé par : amonier	Signé par : vlapere	Signé par : Holowczak Richard	

# INSPECTION REPORT

Customer:

IAA


Page 2/4

+ 0 appendix

Ref.: WS-PVC5893-A

Project Name: SLICER MAAT


File nb: 24906

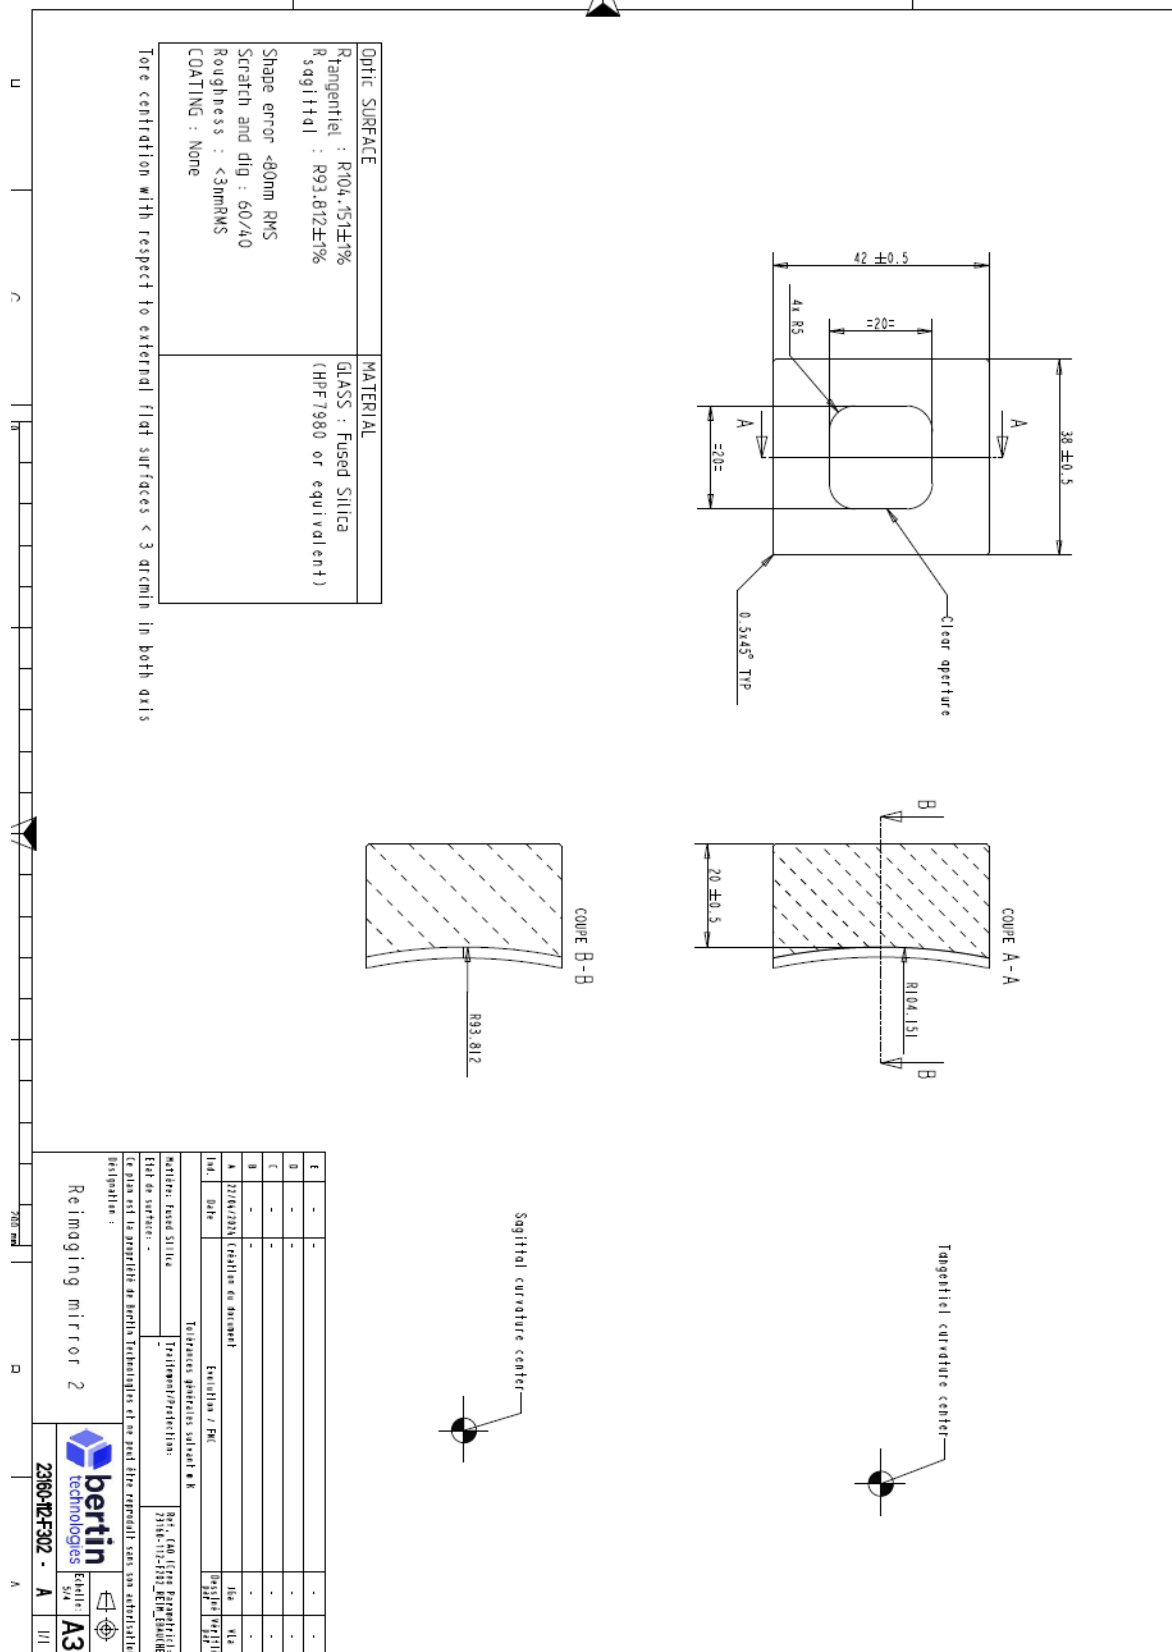


Ref.: WS-PVC5893-A

Project Name: SLICER MAAT

File nb: 24906

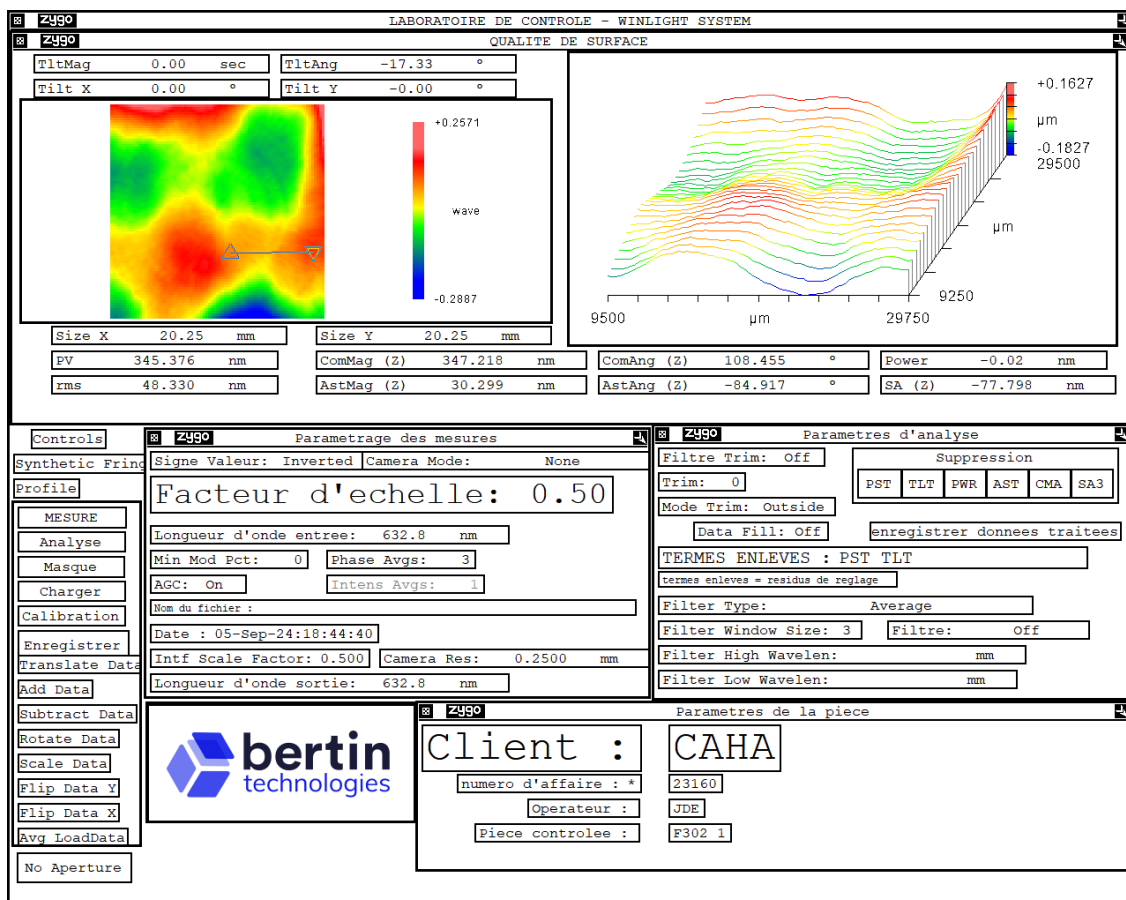

Surface Front Error

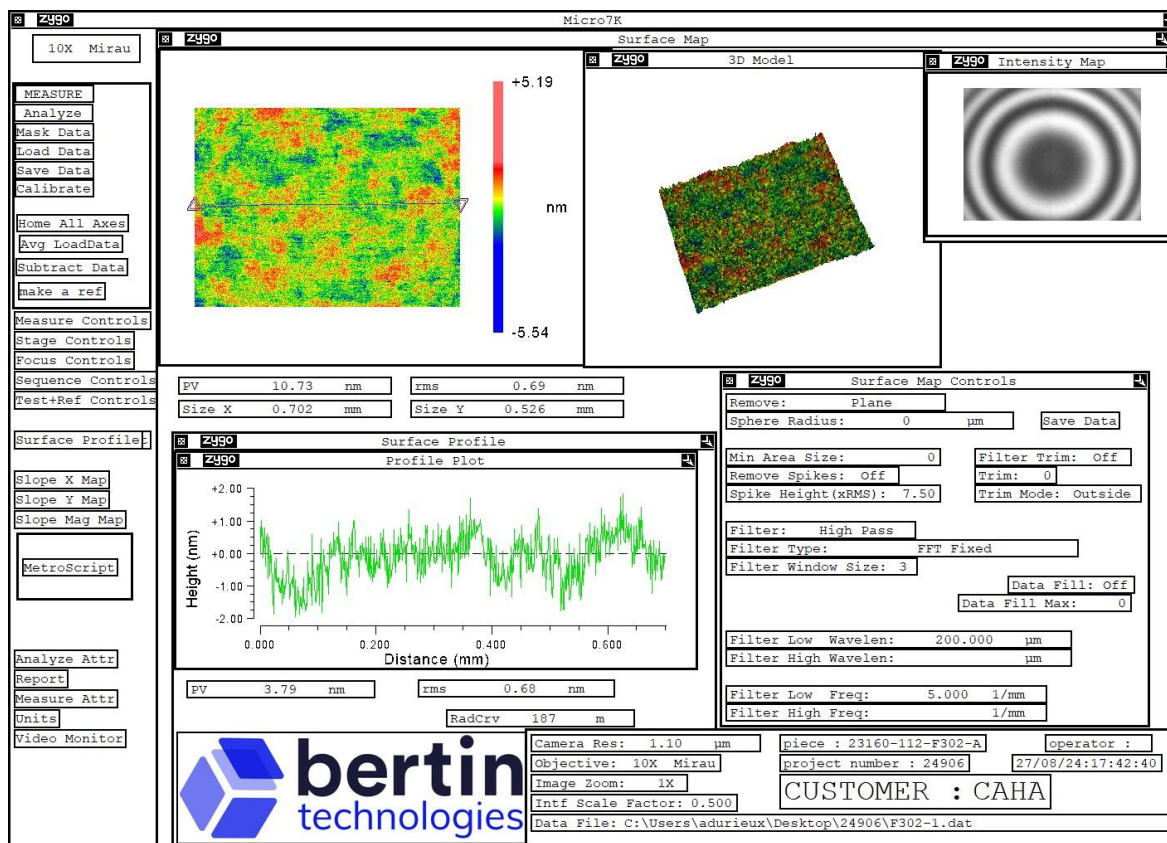

Roughness

# INSPECTION REPORT

Customer:

IAA

Page 4/4

+ 0 appendix

Ref.: WS-PVC5893-A

Project Name: SLICER MAAT

File nb: 24906

## List of measuring tools:

Instrument n°	Instrument designation	Accuracy	Calibration validity date	Reference of the calibration report	Measurement tool used on
WX-APO052	Pied à coulisse 150 mm	± 0,01 mm	25/04/2025	<u>WS-PVE425-A</u>	22/08/2024
WO-APO067	Unité d'affichage + Palpeur Sylvac	Er. Ind.: 3µm Er. Rep.: 1µm	22/10/2024	<u>WS-PVE378-A</u>	22/08/2024
WS-APO027	Nanomefos	Voir PVE	25/10/2024	<u>WS-PVE428-A</u>	05/09/2024
WX-APO001	Rugosimètre 7300 - Zygo NewView	± 0.09 Å RMS	27/03/2025	<u>WS-PVE419-A</u>	27/08/2024
BT-APO002	Stylo optique CHR Mini OEM + sonde -2	± 0,5 mm	24/02/2031	<u>WS-PVE464-A</u>	26/08/2024